


Pitfalls and Errors of HPLC in Pictures

Third, Revised and Enlarged Edition

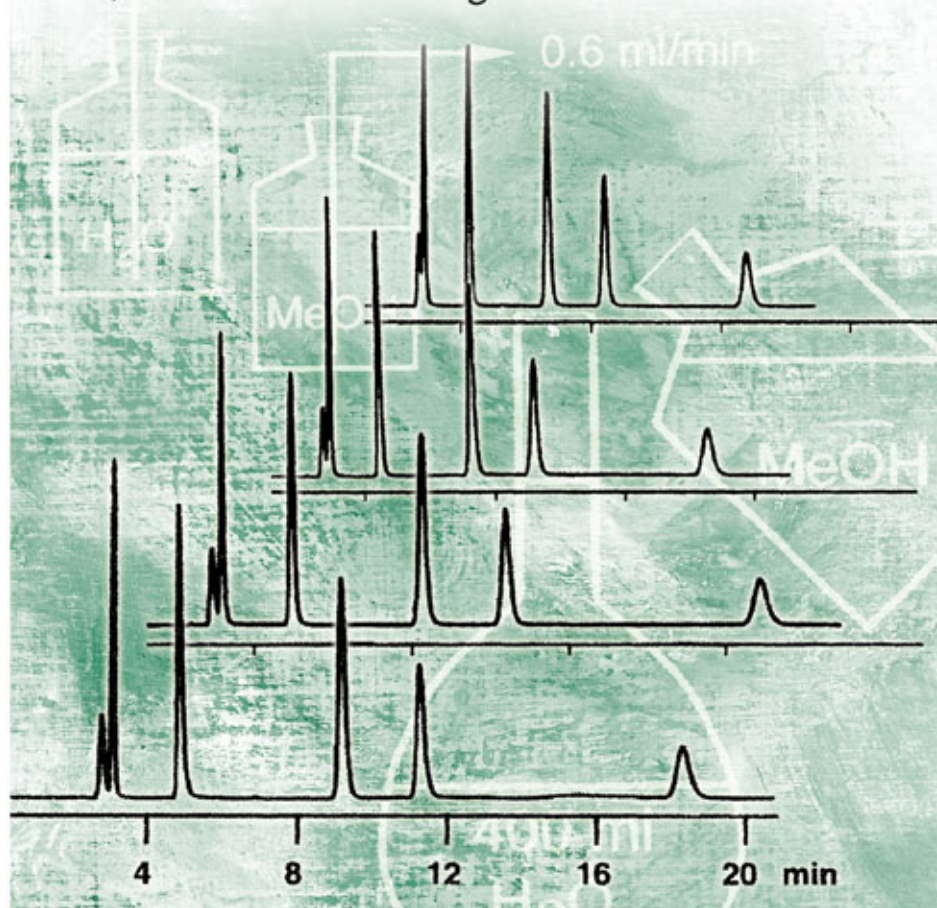

Veronika R. Meyer

Pitfalls and Errors of HPLC in Pictures

Further Titles for Chromatographers

S. Kromidas (ed.)

HPLC Made to Measure

A Practical Handbook for Optimization

2006

ISBN 3-527-31377-X

P. C. Sadek

Troubleshooting HPLC Systems

A Bench Manual

2000

ISBN 0-471-17834-9

S. Kromidas

More Practical Problem Solving in HPLC

2005

ISBN 3-527-31113-0

U. D. Neue

HPLC Columns

Theory, Technology, and Practice

1997

ISBN 0-471-19037-3

V. R. Meyer

Practical High-Performance Liquid Chromatography

2010

ISBN 978-0-470-68218-0 or 978-0-470-68217-3

L. R. Snyder, J. J. Kirkland, J. L. Glajch

Practical HPLC Method Development

1997

ISBN 0-471-00703-X

S. Kromidas

Practical Problem Solving in HPLC

2000

ISBN 3-527-29842-8

Veronika R. Meyer

Pitfalls and Errors of HPLC in Pictures

3., Revised and Enlarged Edition



WILEY-VCH Verlag GmbH & Co. KGaA

The Author

Dr. Veronika R. Meyer

EMPA St. Gallen

Lerchenfeldstrasse 5

9014 St. Gallen

Switzerland

e-mail: veronika.meyer@empa.ch

■ All Books published by **Wiley-VCH** are carefully produced. Nevertheless, editors, authors, and publisher do not warrant the information contained in these books, including this book, to be free of errors. Readers are advised to keep in mind that statements, data, illustrations, procedural details or other items may inadvertently be inaccurate.

Library of Congress Card No.: applied for A catalogue record for this book is available from the British Library.

Bibliographic information published by Die Deutsche Bibliothek

Die Deutsche Bibliothek lists this publication in the Deutsche Nationalbibliografie; detailed bibliographic data is available in the internet at <<http://dnb.ddb.de>>.

© 2013 Wiley-VCH Verlag GmbH & Co. KGaA, Weinheim

All rights reserved (including those of translation into other languages). No part of this book may be reproduced in any form – nor transmitted or translated into a machine language without written permission from the publishers. Registered names, trademarks, etc. used in this book, even when not specifically marked as such, are not to be considered unprotected by law.

Print ISBN: 978-3-527-33293-9

ePDF ISBN: 978-3-527-65913-5

ePub ISBN: 978-3-527-65912-8

mobi ISBN: 978-3-527-65911-1

oBook ISBN: 978-3-527-65910-4

Cover Design Grafik-Design Schulz, Fußgönheim

Typesetting Laserwords Private Ltd., Chennai, India

Printing and Binding Markono Print Media Pte Ltd, Singapore

Printed in Singapore

Printed on acid-free paper

1 wort = 1 millibild

(A picture says more than a thousand words)

Graffiti on the Baltzerstrasse in Bern

Contents

Preface *XI*

Introduction *XIII*

Part I Fundamentals *1*

- 1.1 Chromatography *2*
- 1.2 Chromatographic Figures of Merit *4*
- 1.3 The Resolution of Two Peaks *6*
- 1.4 Reduced Parameters *8*
- 1.5 The Van Deemter Curve *10*
- 1.6 Peak Capacity and Number of Possible Peaks *12*
- 1.7 Statistical Resolution Probability: Simulation *14*
- 1.8 Statistical Resolution Probability: Example *16*
- 1.9 Precision and Accuracy of an Analytical Result *18*
- 1.10 Standard Deviation *20*
- 1.11 Variability of the Standard Deviation *22*
- 1.12 Uncertainty Propagation *24*
- 1.13 Reproducibility in Trace Analysis *26*
- 1.14 Ruggedness *28*
- 1.15 Calibration Curves *30*
- 1.16 The HPLC Instrument *32*
- 1.17 The Detector Response Curve *34*
- 1.18 Noise *36*
- 1.19 The Playground Presented as an Ishikawa Diagram *38*
- 1.20 The Possible and the Impossible *40*

Part II Pitfalls and Sources of Error *43*

- 2.1 Mixing of the Mobile Phase *44*
- 2.2 Mobile Phase pH *46*
- 2.3 Adjustment of Mobile Phase pH *48*
- 2.4 Influence of the Acid Type and Concentration in the Eluent *50*
- 2.5 Water as an Unintentional Additive in the Mobile Phase *52*

2.6	Inadequate Purity of Mobile Phase Water	54
2.7	Inadequate Purity of a Mobile Phase Solvent	56
2.8	Inadequate Purity of a Mobile Phase Reagent	58
2.9	Incomplete Degassing	60
2.10	System Peaks and Quantitative Analysis	62
2.11	Sample Preparation with Solid Phase Extraction	64
2.12	Inadequate Stabilization of the Extraction Solvent	66
2.13	Poor Choice of Sample Solvent: Peak Distortion	68
2.14	Poor Choice of Sample Solvent: Tailing	70
2.15	Sample Solvent and Calibration Curve	72
2.16	Impurities in the Sample	74
2.17	Formation of a By-Product in the Sample Solution	76
2.18	Decomposition by the Sample Vial	78
2.19	Artifact Peaks from the Vial Septum	80
2.20	Formation of an Associate in the Sample Solution	82
2.21	Precision and Accuracy with Loop Injection	84
2.22	Injection Technique	86
2.23	Injection of Air	88
2.24	Sample Adsorption in the Loop	90
2.25	Extra-Column Volumes	92
2.26	Dwell Volume	94
2.27	Elution at t_0	96
2.28	Classification of C_{18} Reversed Phases	98
2.29	Different Selectivity of C_{18} Reversed Phases	100
2.30	Different Batches of Stationary Phase	102
2.31	Chemical Reaction within the Column	104
2.32	Tailing of Phosphate Compounds in the Presence of Steel	106
2.33	Recovery and Peak Shape Problems with Proteins	108
2.34	Double Peaks from Stable Conformers	110
2.35	Influence of Temperature on the Separation	112
2.36	Thermal Non-Equilibrium within the Column	114
2.37	Influence of the Flow Rate on the Separation	116
2.38	Influence of Run Time and Flow Rate on Gradient Separations	118
2.39	UV Spectra and Quantitative Analysis	120
2.40	UV Detection Wavelength	122
2.41	Different Detection Properties of Diastereomers	124
2.42	Fluorescence Quenching by Air	126
2.43	Detector Overload in UV	128
2.44	Detector Overload in ELSD	130
2.45	Influence of the Retention Factor on Peak Height	132
2.46	Influence of the Flow Rate on Peak Area	134
2.47	Leaks in the HPLC Instrument	136
2.48	Impairment of Precision as a Result of Noise	138
2.49	Determination of Peak Area and Height at High Noise	140

2.50	Peak Height Ratios	142
2.51	Incompletely Resolved Peaks	144
2.52	Area Rules for Incompletely Resolved Peaks	146
2.53	Areas of a 1 : 10 Peak Pair	148
2.54	Heights of a 1 : 10 Peak Pair	150
2.55	Quantitative Analysis of a Small Peak	152
2.56	Incompletely Resolved Peaks with Tailing	154
2.57	Integration Threshold and Number of Detected Peaks	156
2.58	Detector Time Constant and Peak Shape	158
2.59	Quantitative Analysis in the 99% Range	160
2.60	Correlation Coefficient of Calibration Curves	162
Part III	Useful Strategies	165
3.1	Column Tests	166
3.2	Apparatus Tests	168
3.3	Wavelength Accuracy of the UV Detector	170
3.4	Internal Standards	172
3.5	A Linearity Test	174
3.6	Rules for Accurate Quantitative Peak Size Determination	176
3.7	High-Low Chromatography	178
3.8	Control Charts	180
3.9	Verification of the Analytical Result by Use of a Second Method	182
3.10	Description of Ruggedness	184
3.11	Rules for Passing On an HPLC Method	186
3.12	Quality Assurance in the Laboratory	188
3.13	Standard Operating Procedures	190
3.14	Method Validation	192
3.15	Some Elements of Validation	194
3.16	A Validation Example	196
3.17	System Suitability Test	198
3.18	From Repeatability to Reproducibility	200
3.19	Measurement Uncertainty	202
3.20	Formal Quality Assurance Systems	204
	Index	207

Preface

Errors are a common companion of all human activity, including work in the laboratory. Yet it is a great pity if erroneous results are produced with great effort and by using expensive instruments and demanding procedures. Therefore a book about sources of errors in high performance liquid chromatography, one of today's most widely used analytical methods, is not superfluous. Maybe the topic is not welcomed enthusiastically but I hope I have found a design which encourages reading and thinking.

In conception, at least, possible problems can be divided into two categories. 'Errors' are troublesome opponents of accurate and precise analytical results which, however, can be understood; we need to remember and to anticipate them. In contrast, 'pitfalls' are totally unexpected intruders and the secret behind them is difficult to discover. The worst are those which are not detected but which affect the result anyway. Nevertheless, the book does not distinguish between the two types. The readers decide how they classify them. With increasing experience in HPLC it should become easier to avoid the pitfalls.

The third edition could be expanded with new examples and proposals. Many people helped me with examples, hints or ideas on how to improve the text and figures. I want to thank all of them. Special thanks to the publisher who supports the idea of a picture book, not for children but for novices and experts in the analytical laboratory. I hope that the book will be a useful aid in daily laboratory work thanks to intelligible explanations and lucid illustrations.

St. Gallen, August 2012

Veronika R. Meyer

Introduction

This book is not an introductory text to HPLC and also not a troubleshooting guide of the kind “what shall I do if my instrument does not work?”. It does not replace such books but is intended to complement them. Some texts which, according to my personal opinion, are very useful and should therefore be present in the HPLC laboratory are listed on the next page.

Now this book on your desk is a picture book. The figures are at least as important as the texts; sometimes more information can be found in them than could be given in the short descriptions. It is possible, and in principle recommended, to study all the pages in sequence from beginning to end. This method guarantees that one learns about errors which are uncommon and unexpected. On the other hand each pair of pages is limited to one topic, linked to other pages by arrows only, and can therefore be studied in isolation. The index at the end of the book can help you find the right pages when a problem occurs, although it must be stated once again that quick troubleshooting advice is not usually provided.

The book is divided into three parts:

Part I briefly presents some basic facts about HPLC. Many topics may be absent because this is not a textbook, but the matter presented is of utmost relevance in HPLC. Thus the topics discussed should act as reminders and be used for revision. Whoever understands Part I knows a lot about HPLC – more than it seems at first glance.

Part II lists the pitfalls and sources of error. They are in a logical sequence, as far as this is possible, following the flow path in an HPLC instrument, from the preparation of the mobile phase to data evaluation. The list is somewhat arbitrary, and not all errors are of equal importance with regard to their possible consequences. It would, however, be dangerous to distinguish between grave and harmless errors. A minute error can cause much damage under special circumstances.

Part III gives some hints on what can be done to avoid errors. Again this synopsis is very heterogeneous in character. This does not diminish its value, of course.

Incompleteness is an inevitable feature of this book. I am grateful for all hints on other pitfalls and sources of error or on how to avoid them.

Recommended Texts

Veronika R. Meyer
Practical High Performance Liquid Chromatography
Wiley, Chichester
5th edition 2010

John W. Dolan and Lloyd R. Snyder
Troubleshooting LC Systems
Humana Press, New Jersey
1989

Paul C. Sadek
Troubleshooting HPLC Systems: A Bench Manual
Wiley-Interscience, New York
2000

Stavros Kromidas
Practical Problem Solving in HPLC
Wiley-VCH, Weinheim
2000

Stavros Kromidas
More Practical Problem Solving in HPLC
Wiley-VCH, Weinheim
2004

Lloyd R. Snyder, Joseph J. Kirkland and Joseph L. Glajch
Practical HPLC Method Development
Wiley-Interscience, New York
2nd edition 1997

Norman Dyson
Chromatographic Integration Methods
Royal Society of Chemistry, London
2nd edition 1998

Part I

Fundamentals

1.1

Chromatography


In chromatography, a physical separation method, the components of a mixture are partitioned between two phases. One of the phases stays in its place and is called the stationary phase, whereas the other moves in a definite direction and is called the mobile phase.

According to the type of mobile phase we distinguish between gas chromatography, supercritical fluid chromatography, and liquid chromatography.

The separation is based upon the different partition coefficients of the sample components between the two phases. It is helpful to divide the chromatographic column into small hypothetical units, the so-called theoretical plates. Within each plate a new partition equilibrium is established. The narrower a theoretical plate, the more equilibrium processes can take place within a column of given length and the more demanding the separation problems which can be solved.

The figure shows the separation of two compounds. One of these prefers the mobile phase but also enters the stationary phase. For the other compound the preference is the other way round. Thanks to this large difference in their properties the two types of molecule can easily be separated. They are transported through the column by the flow of the mobile phase and thereby reach zones where new equilibria are formed again and again.

In the drawing, such a theoretical plate has a height of approximately $3 \frac{1}{2}$ stationary phase particle diameters. This height depends on the packing quality of the column, on the mass transfer properties of the phases, and on the analytes involved. Plate height is a function of the particle diameter of the stationary phase. For good columns, plate heights are equal to ca. 3 particle diameters irrespective of the particle size. A fine packing, e.g. with a $3\text{-}\mu\text{m}$ phase, gives four times as many theoretical plates as does a $10\text{-}\mu\text{m}$ packing if identical column lengths are compared. The column with the fine packing can therefore be used for more difficult separation problems.

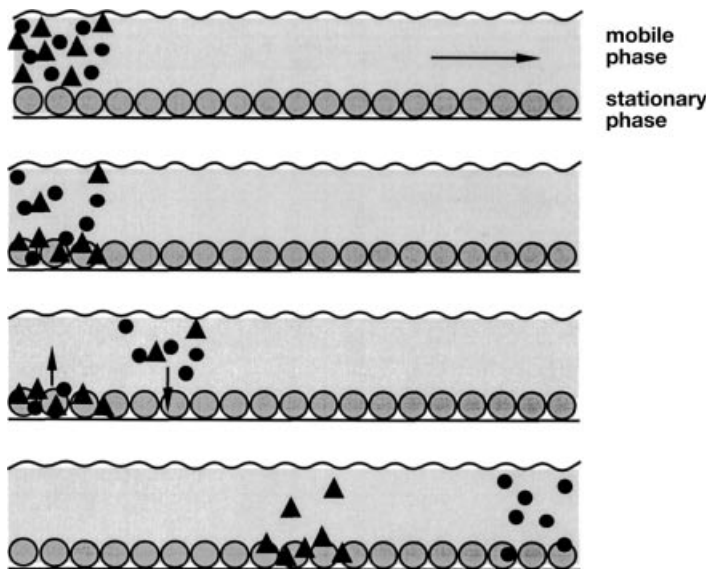

1.2

Chromatographic Figures of Merit

To judge a chromatogram it is necessary to calculate some data which can be easily obtained. The integrator or data system yields the retention times, t_R , and peak widths, w ; perhaps it is advisable to determine the peak width at half height, $w_{1/2}$. In addition the breakthrough time or 'dead time', t_0 , must be known although it can be a problem to measure it unambiguously. In principle, the first baseline deviation after injection marks t_0 . Then the following data can be calculated:

- 1) **Retention factor, k** (formerly capacity factor, k'):

$$k = \frac{t_R - t_0}{t_0}$$

The retention factor is a measure of the retention of a peak. It depends only on the phase system (the types of mobile and stationary phase) and on the temperature.

- 2) **Separation factor, α** :

$$\alpha = \frac{k_2}{k_1}$$

Two compounds can be separated only if α is higher than 1.0 in the selected phase system. For HPLC separations α should be 1.05 or higher ($\rightarrow$ 1.3).

- 3) **Theoretical plate number, N** :

$$N = 16 \left(\frac{t_R}{w} \right)^2 = 5.54 \left(\frac{t_R}{w_{1/2}} \right)^2 = 2\pi \left(\frac{h_P t_R}{A_P} \right)^2$$

where h_P = peak height and A_P peak area. The plate number is a measure of the separation performance of a column. (The equations given here are in principle only valid for symmetrical peaks.)

From the plate number it is possible to calculate the height, H , of a theoretical plate (e.g., in μm):


$$H = \frac{L_c}{N}$$

where L_c = column length.

- 4) **Tailing T** (for asymmetric peaks):

$$T = \frac{b}{a}$$

where a and b are determined at 10% of peak height.

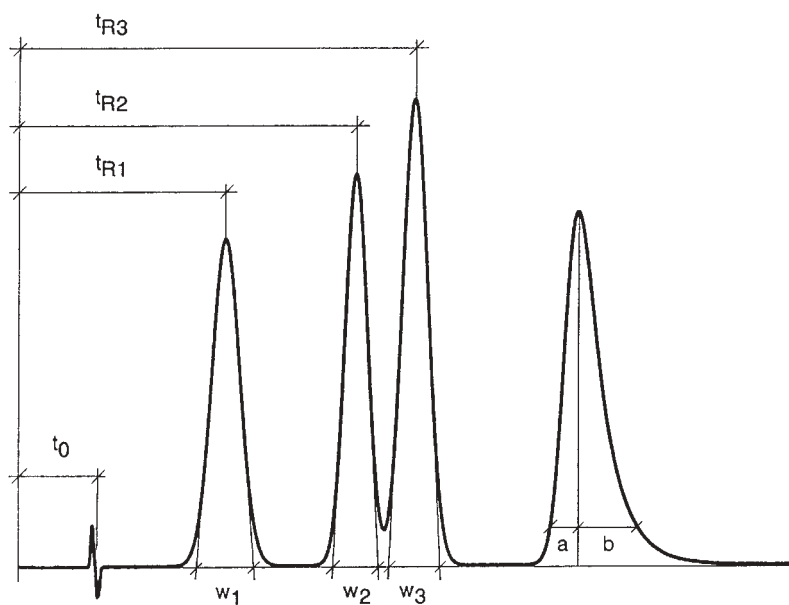

1.3

The Resolution of Two Peaks

The resolution of two adjacent peaks is defined as

$$R = 2 \frac{t_{R2} - t_{R1}}{w_1 + w_2} = 1.18 \frac{t_{R2} - t_{R1}}{w_{1/2_1} + w_{1/2_2}}$$

At a resolution of 1.0 the baseline between the peaks is not reached! Complete resolution is only obtained at $R = 1.5$ or higher, depending on the height ratio of the peaks. The smaller a peak compared with its large neighbor the greater is the resolution necessary to separate them.

The resolution depends on the separation factor α , the theoretical plate number N , and the retention factor k :

$$R = \frac{1}{4} (\alpha - 1) \sqrt{N} \frac{k}{1 + k}$$

This equation can be expressed in different forms, which are not of interest here. It is important to realize that the resolution is influenced by the three parameters. The separation factor has the largest effect. If a separation needs to be improved it is well worth the effort of increasing α , although it is impossible to give a general proposal concerning how to do this. If the plate number is increased, the effect is only by the factor $\sqrt{N}$; if the column length is, e.g., doubled, and by this also the plate number (at least in principle), the resolution will improve only by $\sqrt{2} = 1.4$. Increasing the retention factor only has a notable influence on resolution if k was small to start with.

The upper figure presents several pairs of peaks separated with varying resolution. The graph below demonstrates how the resolution increases with increasing plate number for three different separation factors.