


Edited by Valery V. Tuchin

 WILEY-VCH

Advanced Optical Flow Cytometry

Methods and Disease Diagnoses

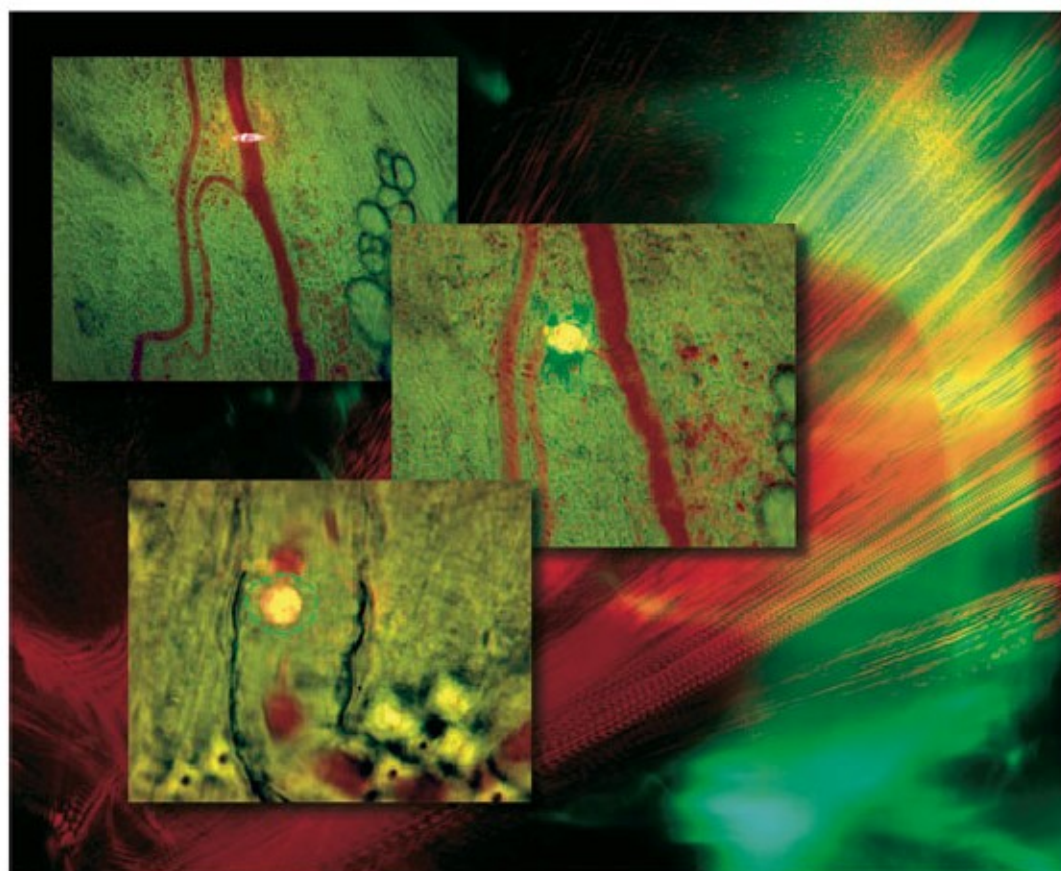

Edited by Valery V. Tuchin

Advanced Optical Flow Cytometry

Related Titles

Lakshmipathy, U., Chesnut, J. D.,
Thyagarajan, B.

Emerging Technology Platforms for Stem Cells

2009
506 pages
Hardcover
ISBN: 978-0-470-14693-4

Wolfbeis, O. S. (ed.)

Fluorescence Methods and Applications Spectroscopy, Imaging, and Probes

2008
452 pages
Softcover
ISBN: 978-1-57331-716-0

Murphy, D. B.

Fundamentals of Light Microscopy and Electronic Imaging

2008
E-Book
ISBN: 978-0-470-24202-5

Prasad, P. N.

Introduction to Biophotonics

2004
E-Book
ISBN: 978-0-471-46539-3

Durack, G., Robinson, J. P. (eds.)

Emerging Tools for Single-Cell Analysis Advances in Optical Measurement Technologies

2002
Online Book Wiley Interscience
ISBN: 978-0-471-22484-6

Givan, A. L.

Flow Cytometry First Principles

296 pages
2001
Softcover
ISBN: 978-0-471-38224-9

Edited by Valery V. Tuchin

Advanced Optical Flow Cytometry

Methods and Disease Diagnoses



**WILEY-
VCH**

WILEY-VCH Verlag GmbH & Co. KGaA

The Editor

Prof. Valery V. Tuchin

Saratov State University
Optics and Biophotonics
Saratov, Russian Federation
tuchinvv@mail.ru

All books published by **Wiley-VCH** are carefully produced. Nevertheless, authors, editors, and publisher do not warrant the information contained in these books, including this book, to be free of errors. Readers are advised to keep in mind that statements, data, illustrations, procedural details or other items may inadvertently be inaccurate.

Library of Congress Card No.: applied for

British Library Cataloguing-in-Publication Data

A catalogue record for this book is available from the British Library.

Bibliographic information published by the Deutsche Nationalbibliothek

The Deutsche Nationalbibliothek lists this publication in the Deutsche Nationalbibliografie; detailed bibliographic data are available on the Internet at <<http://dnb.d-nb.de>>.

© 2011 Wiley-VCH Verlag & Co. KGaA,
Boschstr. 12, 69469 Weinheim,
Germany

All rights reserved (including those of translation into other languages). No part of this book may be reproduced in any form – by photoprinting, microfilm, or any other means – nor transmitted or translated into a machine language without written permission from the publishers. Registered names, trademarks, etc. used in this book, even when not specifically marked as such, are not to be considered unprotected by law.

Cover Design Grafik-Design Schulz,
Fußgönheim

Typesetting Laserwords Private Limited,
Chennai, India

Printing and Binding Strauss GmbH,
Mörtenbach

Printed in the Federal Republic of Germany
Printed on acid-free paper

ISBN: 978-3-527-40934-1

ePDF ISBN: 978-3-527-63430-9

oBook ISBN: 978-3-527-63428-6

ePub ISBN: 978-3-527-63429-3

Mobi ISBN: 978-3-527-63431-6

Contents

Preface XXI

List of Contributors XXXI

1	Perspectives in Cytometry	1
	<i>Anja Mittag and Attila Tárnok</i>	
1.1	Background	1
1.2	Basics of Cytometry	2
1.2.1	Flow Cytometry	2
1.2.2	Slide-Based Cytometry	3
1.3	Cytomics	4
1.4	Cytometry – State of the Art	5
1.4.1	Multiparametric Analyses	6
1.5	Perspectives	7
1.5.1	New Technologies and Methods	10
1.5.1.1	Sequential Analyses	11
1.5.1.2	Spectral Analyses	11
1.5.1.3	Fluorescence Modifications for Analyses	12
1.5.1.4	Label-Free Analyses	13
1.5.2	Automation	14
1.5.3	Cytometry – the Other Side	15
1.6	Conclusion	16
	References	16
2	Novel Concepts and Requirements in Cytometry	25
	<i>Herbert Schneckenburger, Michael Wagner, Petra Weber, and Thomas Bruns</i>	
2.1	Introduction	25
2.2	Fluorescence Microscopy	25
2.2.1	Light Dose	25
2.2.2	Cell Systems	26
2.2.3	Methods	27
2.3	Fluorescence Reader Systems	27
2.3.1	Cell-Based Fluorescence Screening	27

2.3.2	TIR Fluorescence Reader	28
2.4	Microfluidics Based on Optical Tweezers	30
2.5	Conclusion	30
	Acknowledgment	31
	References	31
3	Optical Imaging of Cells with Gold Nanoparticle Clusters as Light Scattering Contrast Agents: A Finite-Difference Time-Domain Approach to the Modeling of Flow Cytometry Configurations	35
	<i>Stoyan Tanev, Wenbo Sun, James Pond, Valery V. Tuchin, and Vladimir P. Zharov</i>	
3.1	Introduction	35
3.2	Fundamentals of the FDTD Method	37
3.2.1	The Basic FDTD Numerical Scheme	37
3.2.2	Input Wave Excitation	39
3.2.3	Uniaxial Perfectly Matched Layer Absorbing Boundary Conditions	39
3.2.4	FDTD Formulation of the Light Scattering Properties from Single Cells	40
3.2.5	FDTD Formulation of Optical Phase Contrast Microscopic (OPCM) Imaging	42
3.3	FDTD Simulation Results of Light Scattering Patterns from Single Cells	45
3.3.1	Effect of Extracellular Medium Absorption on the Light Scattering Patterns	45
3.4	FDTD OPCM Nanobioimaging Simulation Results	47
3.4.1	Cell Structure	47
3.4.2	Optical Clearing Effect	47
3.4.3	The Cell Imaging Effect of Gold Nanoparticles	48
3.4.3.1	A Cell with a Cluster of Gold Nanoparticles Located in the Cytoplasm	50
3.4.3.2	A Cell with a Cluster of Gold Nanoparticles Randomly Distributed on the Surface of its Nucleus	52
3.5	Conclusion	57
	Acknowledgment	59
	References	59
4	Optics of White Blood Cells: Optical Models, Simulations, and Experiments	63
	<i>Valeri P. Maltsev, Alfons G. Hoekstra, and Maxim A. Yurkin</i>	
4.1	Introduction	63
4.1.1	White Blood Cells	63
4.1.2	Particle Identification and Characterization	63
4.1.3	Experimental Techniques	64
4.2	Optical Models of White Blood Cells	65

4.2.1	Confocal Imaging of White Blood Cells	65
4.2.2	Optical Models of Mononuclear Cells	65
4.2.3	Optical Models of Granular Cells	67
4.2.4	Refractive Indices of White Blood Cells and their Organelles	68
4.3	Direct and Inverse Light-Scattering Problems for White Blood Cells	69
4.3.1	Simulation of Light Scattering by Mononuclear Cells	69
4.3.2	Simulation of Light Scattering by Granular Cells	70
4.3.2.1	Granulocyte Model Without Nucleus	70
4.3.2.2	Approximate Theories	72
4.3.2.3	Neutrophil Model with Nucleus	72
4.3.3	Inverse Light-Scattering Problem for Mononuclear Cells	73
4.3.3.1	Global Optimization	74
4.3.3.2	Errors of Parameter Estimates	74
4.3.3.3	Theoretical Tests Based on More Complicated Model	76
4.3.3.4	Sample Characterization	77
4.4	Experimental Measurement of Light Scattering by White Blood Cells	78
4.4.1	Scanning Flow Cytometer	78
4.4.1.1	The Current State of the Art of the SFC	79
4.4.1.2	Mueller Matrix of the SFC	80
4.4.2	Differential Scattering Cross Section of White Blood Cells	81
4.4.3	Measurement of Light Scattering of Mononuclear Cells	82
4.4.4	Characterization of Mononuclear Cells from Light Scattering	84
4.4.5	Measurement of Light Scattering of Granular Cells	87
4.5	Conclusion	89
	Acknowledgments	90
	References	90
5	Optical Properties of Flowing Blood Cells	95
	<i>Martina C. Meinke, Moritz Friebe, and Jürgen Helfmann</i>	
5.1	Introduction	95
5.2	Blood Physiology	96
5.2.1	Blood Composition	96
5.2.2	Clinical Parameters	98
5.2.3	Physiological Conditions	99
5.3	Complex Refractive Index of Hemoglobin	100
5.4	Light Propagation in Turbid Media	102
5.4.1	Monte Carlo Simulation	104
5.5	Method for the Determination of Optical Properties of Turbid Media	104
5.5.1	Integrating Sphere Measurements	104
5.5.2	Principle of Inverse Monte Carlo Simulation	106

5.5.3	Possibility of Determining the Intrinsic Parameters	107
5.5.4	Preparation of the Blood Samples	108
5.5.4.1	Red Blood Cells	108
5.5.4.2	Plasma	108
5.5.4.3	Platelets	109
5.6	Optical Properties of Red Blood Cells	109
5.6.1	Standard Red Blood Cells	110
5.6.2	Optical Parameters of Red Blood Cells Dependent on Hematocrit	112
5.6.3	Influence of Oxygen Saturation	115
5.6.4	Influence of Shear Rate	117
5.6.4.1	Shear Rate Range 0–200 s ⁻¹	118
5.6.4.2	Shear Rate Range 200–600 s ⁻¹	119
5.6.4.3	Shear Rates at 1000 s ⁻¹	119
5.6.5	Influence of Osmolarity	119
5.7	Optical Properties of Plasma	122
5.7.1	Influence of the Surrounding Medium on Red Blood Cells	124
5.8	Optical Properties of Platelets	126
5.9	Comparison of Optical Influences Induced by Physiological Blood Parameters	127
5.10	Summary	129
	Acknowledgments	129
	References	129

6 Laser Diffraction by the Erythrocytes and Deformability Measurements

Sergei Yu. Nikitin, Alexander V. Priezzhev, and Andrei E. Lugovtsov

6.1	Introduction	133
6.2	Parameters of the Erythrocytes	134
6.3	Parameters of the Ektacytometer	135
6.4	Light Scattering by a Large Optically Soft Particle	136
6.5	Fraunhofer Diffraction	138
6.6	Light Scattering by a Transparent Elliptical Disc	140
6.7	Light Scattering by an Elliptical Disc with Arbitrary Coordinates of the Disc Center	143
6.8	Light Diffraction by an Ensemble of Particles	144
6.9	Light Diffraction by Particles with Random Coordinates	145
6.10	Light Scattering by Particles with Regular Coordinates	146
6.11	Description of the Experimental Setup	147
6.12	Sample Preparation Procedure	149
6.13	Examples of Experimental Assessment of Erythrocyte Deformability in Norm and Pathology	150
6.14	Conclusion	153
	References	153

7	Characterization of Red Blood Cells' Rheological and Physiological State Using Optical Flicker Spectroscopy	155
	<i>Vadim L. Kononenko</i>	
7.1	Introduction	155
7.2	Cell State-Dependent Mechanical Properties of Red Blood Cells	156
7.3	Flicker in Erythrocytes	158
7.3.1	Phenomenology of Cell Membrane Flickering	159
7.3.2	Theoretical Models of Flicker	160
7.3.2.1	Models with Various Cell Shape under Thermal Excitation	162
7.3.2.2	Flat Disk Model	166
7.3.2.3	Active Excitation Mechanisms	171
7.4	Experimental Techniques for Flicker Measurement in Blood Cells	173
7.4.1	Measurement of Frequency Spectra of Membrane Flickering	173
7.4.1.1	Phase Contrast and Laser Probing of Central Part of Erythrocyte Disk	173
7.4.1.2	Point Probing of Cell Edge Fluctuations	178
7.4.2	Quantitative Phase Imaging of Entire Cell	179
7.4.3	Registration of Fluctuations in Cell Circumference Shape	182
7.4.4	Fundamental Difference between the Registered Spectra and the Intrinsic Flicker Spectrum	183
7.5	The Measured Quantities in Flicker Spectroscopy and the Cell Parameters Monitored	187
7.5.1	Frequency Spectra	187
7.5.1.1	Disk Face Area of Erythrocyte	187
7.5.1.2	Equatorial Contour and Rim Area	188
7.5.2	Modal Composition	189
7.5.2.1	Disk Face Area of Erythrocyte	189
7.5.2.2	Equatorial Contour	191
7.5.3	Mean Square Amplitude Distribution	191
7.6	Flicker Spectrum Influence by Factors of Various Nature	192
7.6.1	Ambient Physical Conditions	193
7.6.1.1	Effect of Medium Viscosity	193
7.6.1.2	Effect of Ambient Temperature	194
7.6.1.3	Effect of Medium Tonicity	195
7.6.2	Modification of Cell Mechanical Properties	197
7.6.3	Physiologically Active Substances and Medicinal Drugs	198
7.6.4	Erythrocyte Flicker at Human Pathologies	200
7.7	Membrane Flicker and Erythrocyte Functioning	201
7.8	Flicker in Other Cells	203
7.9	Conclusions	204
	References	205

8	Digital Holographic Microscopy for Quantitative Live Cell Imaging and Cytometry	211
	<i>Björn Kemper and Jürgen Schnekenburger</i>	
8.1	Introduction, Motivation, and Background	211
8.2	Principle of DHM	212
8.2.1	DHM Setup and Imaging	212
8.2.2	Evaluation of Digital Holograms	213
8.2.3	Quantitative Phase Contrast Imaging and Cell Thickness Determination	216
8.2.4	DHM Multifocus Imaging and Cell Tracking	217
8.3	DHM in Cell Analysis	221
8.3.1	Cell Cultures	222
8.3.2	DHM Cell Thickness Measurements	223
8.3.3	Dynamic Cell Thickness Monitoring in Toxicology	224
8.3.4	Label-Free Detection of Apoptotic Processes	227
8.3.5	Determination of the Integral Refractive Index of Cells in Suspension	228
8.3.6	Identification of Subcellular Structures	232
8.4	Conclusion	234
	Acknowledgment	234
	References	234
9	Comparison of Immunophenotyping and Rare Cell Detection by Slide-Based Imaging Cytometry and Flow Cytometry	239
	<i>József Bocsi, Anja Mittag, and Attila Tárnok</i>	
9.1	Introduction	239
9.1.1	Cytometry of Equal Quality?	240
9.1.2	Fluorescence Analyses	240
9.1.2.1	Excitation and Emission of Fluorescent Dyes	240
9.1.2.2	Quantum Dots	241
9.1.2.3	Bleaching Characteristics of Dyes	243
9.1.2.4	Fluorescent Light Detection	243
9.1.2.5	Spillover Characteristics	244
9.1.3	Two Ways of Cytometric Analysis	244
9.1.3.1	Flow Cytometry	244
9.1.3.2	Slide-Based Cytometry	246
9.2	Comparison of Four-Color CD4/CD8 Leukocyte Analysis by SFM and FCM Using Qdot Staining	247
9.2.1	Analysis of Lymphocytes by SFM and FCM	247
9.2.2	Comparison of CD4/CD8 Ratio	248
9.3	Comparison of Leukocyte Subtyping by Multiparametric Analysis with LSC and FCM	250
9.3.1	Different Triggering in LSC Analysis	250
9.3.2	Immunophenotyping by FCM and LSC	254
9.3.3	Multicolor Analyses	256

9.4	Absolute and Relative Tumor Cell Frequency Determinations	256
9.4.1	Comparison of Cell Counts	257
9.4.1.1	Dilution Series	257
9.4.1.2	Rare Cell Analysis	259
9.4.2	Analysis Documentation	259
9.4.3	Limitations	261
9.5	Analysis of Drug-Induced Apoptosis in Leukocytes by Propidium Iodide	262
9.5.1	Induction of Apoptosis	263
9.5.2	Apoptosis Detection by SBC and FCM	265
9.6	Conclusion	266
	Acknowledgment	266
	References	266
10	Microfluidic Flow Cytometry: Advancements toward Compact, Integrated Systems	273
	<i>Shawn O. Meade, Jessica Godin, Chun-Hao Chen, Sung Hwan Cho, Frank S. Tsai, Wen Qiao, and Yu-Hwa Lo</i>	
10.1	Introduction	273
10.1.1	Main Components of a Full-Scale Flow Cytometer	273
10.1.1.1	Fluidic Control System	273
10.1.1.2	Optical Detection System	274
10.1.1.3	Sorting Modules	274
10.1.2	Microfluidic Flow Cytometry	275
10.2	On-Chip Flow Confinement	275
10.2.1	A General Discussion of Flow Confinement Forces	276
10.2.2	Two-Dimensional Flow Confinement	277
10.2.3	Three-Dimensional Flow Confinement	278
10.3	Optical Detection System	283
10.3.1	The Many Benefits of Integrated Optics	283
10.3.2	Developing the Tools of the Trade	284
10.3.2.1	Light-Guiding Elements	284
10.3.2.2	Two-Dimensional Refractive Elements	286
10.3.2.3	Improving Quality of On-Chip Optics	288
10.3.2.4	Light-Stopping and Reflecting Elements	290
10.3.2.5	Spectral Separation	290
10.3.2.6	Tunable Liquid-Core Waveguides and Lenses	290
10.3.3	Opportunities for Significant Improvements over Bulk Optical Systems	292
10.4	On-Chip Sorting	297
10.4.1	Electrokinetic Sorting	297
10.4.2	Sorting by Dielectrophoresis	298
10.4.3	Sorting by Optical Force	299
10.4.4	Hydrodynamic Sorting	300
10.4.4.1	Hydrodynamic Sorting with External Check Valves	301

10.4.4.2	Hydrodynamic Sorting with Piezoelectric Actuators	301
10.5	Conclusion	306
	Acknowledgments	306
	References	306
11	Label-Free Cell Classification with Diffraction Imaging Flow Cytometer	311
	<i>Xin-Hua Hu and Jun Q. Lu</i>	
11.1	Introduction	311
11.2	Modeling of Scattered Light	313
11.2.1	The Correlation between Scattered Light Distribution and Cellular Structure	314
11.2.2	The Formulation of Stokes Vector and Muller Matrix	316
11.3	FDTD Simulation with 3D Cellular Structures	318
11.3.1	The FDTD Algorithm	318
11.3.2	Acquisition of 3D Cell Structure through Confocal Imaging	321
11.4	Simulation and Measurement of Diffraction Images	322
11.4.1	Numerical Results Based on FDTD Simulations	323
11.4.2	Experimental Results Acquired with a Diffraction Imaging Flow Cytometer	325
11.5	Summary	327
	Acknowledgments	328
	References	328
12	An Integrative Approach for Immune Monitoring of Human Health and Disease by Advanced Flow Cytometry Methods	333
	<i>Rabindra Tirouvanziam, Daisy Diaz, Yael Gernez, Julie Laval, Monique Crubezy, and Megha Makam</i>	
12.1	Introduction	333
12.2	Optimized Protocols for Advanced Flow Cytometric Analysis of Human Samples	335
12.2.1	Key Limitations of Current Experimental Approaches: Technical and Scientific Biases	335
12.2.2	Developing Better Protocols for Flow Cytometry Studies of Cells from Human Subjects: Enabling Holistic Studies of Human Health and Disease	336
12.2.3	Integrating Flow Cytometry into a Wider Framework for Experimental Research on Human Samples	339
12.3	Reagents for Advanced Flow Cytometric Analysis of Human Samples	341
12.3.1	Antibody Probes	341
12.3.2	Nonantibody Probes	347
12.3.3	Adapting Protocols to the Research Question at Hand: A Few Practical Examples	352

- 12.4 Conclusion: The Future of Advanced Flow Cytometry in Human Research 355
 Acknowledgments 359
 Abbreviations 359
 References 360
- 13 Optical Tweezers and Cytometry 363**
Raktim Dasgupta and Pradeep Kumar Gupta
- 13.1 Introduction 363
- 13.2 Optical Tweezers: Manipulating Cells with Light 364
- 13.2.1 Basics Principles 364
- 13.2.2 Experimental Considerations 366
- 13.3 Use of Optical Tweezers for the Measurement of Viscoelastic Parameters of Cells 367
- 13.3.1 Red Blood Cells 368
- 13.3.1.1 Use of Multiple Optical Traps 369
- 13.3.1.2 Use of Counterpropagating Light Beams 372
- 13.3.1.3 Use of Evanescent Wave of Light 373
- 13.3.1.4 Use of Viscous Drag on Optically Trapped Cell 373
- 13.3.2 Cancer Cells 374
- 13.3.3 Stem Cells 376
- 13.4 Cytometry with Raman Optical Tweezers 376
- 13.4.1 Raman Optical Tweezers: Basics 376
- 13.4.2 Cytometry Applications 378
- 13.4.2.1 Real-Time Study of Dynamic Processes in Single Cell 378
- 13.4.2.2 Identification and Sorting of Microorganism 379
- 13.4.2.3 Studies on Disease Diagnosis 381
- 13.5 Cell Sorting 381
- 13.6 Summary 383
 References 383
- 14 *In vivo* Image Flow Cytometry 387**
Valery V. Tuchin, Ekaterina I. Galanzha, and Vladimir P. Zharov
- 14.1 Introduction 387
- 14.2 State of the Art of Intravital Microscopy 388
- 14.2.1 General Requirements 388
- 14.2.2 Intravital Video Microscopy (IVM) 389
- 14.2.3 Fluorescent Intravital Video Microscopy (FIVM) 389
- 14.2.4 Experimental Preparations for IVM: Animal Models 390
- 14.2.5 Microcirculation and Cell Flow Examination 392
- 14.2.5.1 Microcirculation and Cell Flow 392
- 14.2.5.2 Light Microscopy 392
- 14.2.5.3 High-Resolution High-Speed Transmission Digital Microscopy (TDM) 393
- 14.2.5.4 Monitoring of Cells in Lymph Flow 395

14.2.5.5	Fluorescent Image Microscopy	396
14.2.5.6	Laser Scanning Microscopy	397
14.2.5.7	Laser Doppler Perfusion Imaging and Laser Speckle Contrast Imaging	399
14.2.5.8	Other Intravital Techniques	400
14.2.5.9	Conclusion	401
14.3	<i>In vivo</i> Lymph Flow Cytometry	401
14.3.1	Basic Idea: Natural Cell-Focusing Phenomenon	401
14.3.2	Animal Model and Experimental Arrangement	402
14.3.3	Lymph Flow Velocity Measurements	406
14.3.4	Imaging of Cells and Lymphatic Structures	409
14.3.5	Summary	415
14.4	High-Resolution Single-Cell Imaging in Lymphatics	415
14.4.1	The High-Speed TDM	415
14.4.2	Optical Clearing for <i>In vivo</i> Label-Free Image Cytometry	417
14.5	<i>In vivo</i> Blood Flow Cytometry	418
14.5.1	The Specificity of Blood Flow Cytometry	418
14.5.2	The High-Speed, High-Resolution Imaging Blood Flow Cytometry	421
14.5.3	The Limitations and Future Perspectives	422
14.5.4	Summary	423
14.6	Conclusion	424
	Acknowledgments	424
	References	425
15	Instrumentation for <i>In vivo</i> Flow Cytometry – a Sickle Cell Anemia Case Study	433
	<i>Stephen P. Morgan and Ian M. Stockford</i>	
15.1	Introduction	433
15.2	Clinical Need	434
15.3	Instrumentation	435
15.3.1	Illumination Methods	435
15.3.1.1	Orthogonal Polarization Spectral Imaging (OPS)	436
15.3.1.2	Dark Field Epi-illumination (DFEI)	437
15.3.1.3	Sidestream Dark Field (SSDF) Illumination	438
15.3.2	Detection	439
15.3.2.1	Custom-Made CMOS Sensors	442
15.4	Image Processing	444
15.5	Modeling	447
15.5.1	Model Description	447
15.5.2	Comparison of Illumination Techniques (DFEI, OPS, and SSDF)	450
15.5.2.1	Proportion of “Useful” Photons	450
15.5.2.2	Imaging Performance	453
15.6	Device Design – Sickle Cell Anemia Imaging System	453

15.7	Imaging Results – Sick Cell Anemia Imaging System	455
15.8	Discussion and Future Directions	458
	References	459
16	Advances in Fluorescence-Based <i>In vivo</i> Flow Cytometry for Cancer Applications	463
	<i>Cherry Greiner and Irene Georgakoudi</i>	
16.1	Introduction	463
16.2	Background: Cancer Metastasis	464
16.3	Clinical Relevance: Role of CTCs in Cancer Development and Response to Treatment	466
16.3.1	Detection and Enumeration of Circulating Non-Epithelial Cancer Cells	467
16.4	Current Methods	468
16.4.1	Enrichment Techniques	468
16.4.2	Detection Techniques	470
16.4.3	Summary	474
16.5	<i>In vivo</i> Flow Cytometry (IVFC)	474
16.6	Single-Photon IVFC (SPIVFC)	477
16.6.1	Principles, Advantages, and Limitations	477
16.6.2	Instrumentation	480
16.6.2.1	Two-Color SPIVFC	480
16.6.2.2	Imaging IVFC	482
16.6.2.3	Retinal Flow IVFC	482
16.6.3	Applications in Enumeration of CTCs	483
16.7	Multiphoton IVFC (MPIVFC)	485
16.7.1	Principles, Advantages, and Limitations	485
16.7.2	Instrumentation	487
16.7.2.1	Two-Color and Extended Laser MPIVFC	487
16.7.2.2	Two-Beam MPIVFC	489
16.7.2.3	Fiber-Based MPIVFC	489
16.7.3	Applications in Enumeration of CTCs	490
16.8	Summary and Future Directions	492
	Acknowledgments	495
	References	495
17	<i>In vivo</i> Photothermal and Photoacoustic Flow Cytometry	501
	<i>Valery V. Tuchin, Ekaterina I. Galanzha, and Vladimir P. Zharov</i>	
17.1	Introduction	501
17.2	Photothermal and Photoacoustic Effects at Single-Cell Level	502
17.2.1	Basic Principles	502
17.2.2	Signal Description	505
17.3	PT Technique	507
17.3.1	PT Spectroscopy	507
17.3.2	PT Scanning Image Cytometry	508

- 17.3.3 PT Flow Cytometry (PTFC) 508
- 17.3.3.1 PT Image Flow Cytometry 508
- 17.3.3.2 PTFC System and Its Image Resolution 511
- 17.3.3.3 PTFC with Thermal-Lens Mode 514
- 17.3.3.4 PTFC Integrating Thermal-Lens and Imaging Modes 515
- 17.4 Integrated PTFC for *In vivo* Studies 518
- 17.4.1 General Schematics of the Instrument 518
- 17.4.2 High-Resolution Imaging of Flowing Cells 521
- 17.4.3 PT Identification of Cells 523
- 17.4.4 Cell Targeting with Gold Nanoparticles 523
- 17.5 Integrated PAFC for *In vivo* Studies 524
- 17.5.1 Schematics of the Instrument 524
- 17.5.2 Animal Models 526
- 17.5.3 Contrast Agents for PAFC 526
- 17.5.4 PAFC Testing and Applications 528
- 17.5.4.1 Testing on Noninvasiveness 528
- 17.5.4.2 PAFC Testing Using Vital Dyes 528
- 17.5.4.3 PAFC Detection of Circulating Nanoparticles 530
- 17.5.4.4 PA Detection of Single Circulating Bacteria 533
- 17.5.4.5 PAFC Benefits and Potentialities 537
- 17.6 *In vivo* Lymph Flow Cytometry 539
- 17.6.1 Principles and Main Applications of Lymph FC 539
- 17.6.1.1 Schematics of Integrated Lymph FC 539
- 17.6.1.2 Label-Free Counting of Metastatic Melanoma Cells 541
- 17.6.1.3 Label-Free PA Detection of Lymphocytes 542
- 17.6.1.4 Real-Time Two-Wavelength Lymph FC with Multicolor Probes 543
- 17.6.2 High-Resolution Single-Cell Imaging 543
- 17.6.2.1 High-Speed Imaging 543
- 17.6.2.2 Capability of Multimodal Cell Imaging 544
- 17.6.2.3 Conclusion Remarks 546
- 17.7 *In vivo* Mapping of Sentinel Lymph Nodes (SLNs) 547
- 17.7.1 Motivation for Cancer Prognoses 547
- 17.7.2 Fiber-Based Multimodal Diagnostic-Therapeutic Platform 548
- 17.7.2.1 Experimental Arrangement and Methodology 548
- 17.7.2.2 Contrasting Agents, Cells under Study, and Animal Model 549
- 17.7.3 *In vivo* and *In vitro* SLN Studies 550
- 17.7.3.1 SLN Examination 550
- 17.7.3.2 Two-Wavelength PA Lymphography with Multicolor Nanoparticles 550
- 17.7.3.3 Melanoma Model: Detection of Tumor Cells in Lymphatics and SLNs 551
- 17.7.3.4 PA Detection of Breast Cancer Metastases in SLNs with Functionalized Nanoparticles 552
- 17.7.3.5 Targeted Laser PT Purging Metastases in a SLN 554
- 17.7.4 Discussion of PA/PT Platform Benefits and Perspectives 556

17.8	Concluding Remarks and Discussion	558
	Acknowledgments	563
	References	563
18	Optical Instrumentation for the Measurement of Blood Perfusion, Concentration, and Oxygenation in Living Microcirculation	573
	<i>Martin J. Leahy and Jim O'Doherty</i>	
18.1	Introduction	573
18.2	Xe Clearance	577
18.3	Naifold Capillaroscopy	577
18.3.1	Data Analysis	579
18.3.2	Applications	580
18.3.3	Limitations and Improved Analysis	581
18.4	LDPM/LDPI	582
18.4.1	Principles of Operation of LDPI	582
18.5	Laser Speckle Perfusion Imaging (LSPI)	583
18.6	TiVi	584
18.6.1	Principles of Operation of TiVi	584
18.7	Comparison of TiVi, LSPI, and LDPI	586
18.7.1	Laser Doppler Imaging – Moor Instruments – MoorLDLS	586
18.7.2	Laser Speckle Imaging – Moor Instruments – MoorFLPI	587
18.7.3	Polarization Spectroscopy – Wheels Bridge – Tissue Viability TiVi Imager	588
18.7.4	Comparison of Imaging Systems	588
18.7.5	Discussion	590
18.8	Pulse Oximetry	592
18.8.1	Historical and Literature Review	592
18.8.2	Alternative Methods for Measurement of Oxygenation	595
18.8.3	Transcutaneous Oxygen Pressure (TCpO ₂)	595
18.8.4	Near Infrared Spectroscopy (NIRS)	596
18.8.5	Luminescence Quenching (Fluorescence and Phosphorescence)	597
18.9	Conclusions	597
	Acknowledgments	598
	References	599
19	Blood Flow Cytometry and Cell Aggregation Study with Laser Speckle	605
	<i>Qingming Luo, Jianjun Qiu, and Pengcheng Li</i>	
19.1	Introduction	605
19.2	Laser Speckle Contrast Imaging	605
19.2.1	Fundamentals	605
19.2.2	Instrumentation	607
19.3	Investigation of Optimum Imaging Conditions with Numerical Simulation	608
19.3.1	Static Speckle Field Simulation	608

19.3.2	Dynamic Speckle Field Simulation	610
19.3.3	Speckle Size and Speckle Contrast	611
19.3.4	Specificities of CCD Camera and Speckle Contrast	612
19.4	Spatio-Temporal Laser Speckle Contrast Analysis	614
19.4.1	Spatial Based Method	614
19.4.2	Temporal Based Method	615
19.4.3	Spatio-Temporal Based Method	615
19.4.4	Theoretical and Experimental Comparisons	616
19.5	Fast Blood Flow Visualization Using GPU	618
19.5.1	CPU-Based Solutions for LSCI Data Processing	618
19.5.2	GPU-Based Solution for LSCI Data Processing	620
19.6	Detecting Aggregation of Red Blood Cells or Platelets Using Laser Speckle	621
19.7	Conclusion	623
	Acknowledgments	624
	References	624
20	Modifications of Optical Properties of Blood during Photodynamic Reactions <i>In vitro</i> and <i>In vivo</i>	627
	<i>Alexandre Douplik, Alexander Stratonnikov, Olga Zhernovaya, and Viktor Loshchenov</i>	
20.1	Introduction	627
20.2	Description and Brief History of PDT	627
20.3	PDT Mechanisms	628
20.4	Blood and PDT	632
20.5	Properties of Blood, Blood Cells, and Photosensitizers: Before Photodynamic Reaction	633
20.5.1	Main Physiological Properties of Blood (Hematocrit, Hemoglobin, Oxygenation, Share Rate) Coupled with Its Absorption, Scattering, and Autofluorescence	633
20.5.2	Blood and Blood Component Autofluorescence	637
20.5.3	Overview of Optical Properties of Contemporary Photosensitizers Used for Systemic Administration	638
20.5.4	Interaction of Photosensitizers with Blood Cells: Uptake Locations and Pharmacokinetics	641
20.5.5	Alteration of the Optical Properties of the Photosensitizers Dissolved in Blood	642
20.6	Photodynamic Reactions in Blood and Blood Cells, Blood Components, and Cells	651
20.6.1	Photodynamic Modifications and Alterations of Blood Plasma and Plasma Proteins	651
20.6.2	Photodynamic Modifications and Alterations of Red Blood Cells (Erythrocytes)	651
20.6.3	Photodynamic Modifications and Alterations of White Blood Cells (Leucocytes)	654

20.6.4	Photodynamic Modifications and Alterations of Blood Platelets (Thrombocytes) 654
20.7	Types of Photodynamic Reactions in Blood: <i>In vitro</i> versus <i>In vivo</i> 656
20.8	Blood Sample <i>In vitro</i> as a Model Studying Photodynamic Reaction 658
20.8.1	Blood Heating Effects during PDT <i>In vitro</i> 660
20.8.2	Monitoring of Oxygen Consumption, Photosensitizer Concentration, and Fluence Rate during Photodynamic Therapy in Whole Blood and Individual Blood Cells 661
20.8.3	Theoretical Model of Oxygen Consumption and Photobleaching in Blood during PDT <i>In vitro</i> 670
20.9	Monitoring of Oxygen Consumption and Photobleaching in Blood during PDT <i>In vivo</i> 677
20.10	Photodynamic Disinfection of Blood 679
20.11	Photodynamic Therapy of Blood Cell Cancer 682
20.12	Summary 685
	Acknowledgments 686
	Glossary 686
	References 687
	Index 699

Preface

Flow cytometry was invented in the late 1960s, and since then the flow cytometer has become an indispensable tool in modern research and clinical laboratories [1–7]. Beyond the routine usage, new trends can be observed in the development of flow cytometric techniques. The main technological improvements include high-speed sorting, phase-sensitive flow cytometry, multicolor flow cytometry, high-throughput multiplex bead assays, and spectral detection, and it provides the basis for extensive data collection.

Classical flow cytometry (FC) uses an instrument system for making, processing, and displaying one or more measurements on individual cells in flowing cell suspension [1–7]. Cells may be stained with one or more fluorescent dyes specific to cell components of interest, for example, DNA, and fluorescence of each cell is measured as cells one by one rapidly transverse the excitation beam (laser or mercury arc lamp). Fluorescence provides a quantitative measure of various biochemical and biophysical properties of the cell. Other measurable optical parameters, which are applicable to the measurement of cell size, shape, density, granularity, and stain uptake, include light absorption, light scattering, and polarization degree.

Numerous clinical and research applications, especially in anatomic pathology for detection and study of malignant lesions, use the so-called image cytometry. This technique encompasses morphometry and densitometry as measuring techniques, and neural networks and expert systems for processing of collected data.

Another cytometric technique is the microscope-based *laser scanning cytometry*, which allows one to make fluorescence measurements and topographic analysis on individual cells. Laser-induced fluorescence of labeled cellular specimens is detected using multiple discrete wavelengths, and the spatially resolved data are processed to quantify cell proliferation, apoptosis, gene expression, protein transport, and other cellular processes. For instance, confocal microscopy and two-photon imaging techniques are able to detect fluorescently labeled cells not only *in vitro* but also *in vivo* [8].

Improvements in image cytometric techniques speeded up in the last two decades, applying more and more sensitive detectors and introducing nonlinear optics (two photon excitation) for lifetime measurements (fluorescence lifetime imaging microscopy, FLIM). The latest developments were able to break the

diffraction limit as in the scanning near-field optical microscopy (SNOM), total internal reflection microscopy (TIRFM), fluorescence resonance energy transfer (FRET), stimulated emission depletion (STED), and 4Pi and multiobjective microscopy.

Conventional FC is currently the method of choice for rapid quantification of cells, but it requires invasive extraction of cells from a living organism and associated procedures (e.g., fluorescence labeling and sorting), which may lead to unpredictable artifacts, and prevents long-term cell monitoring in the native biological environment. Among *in vivo* techniques, both nonoptical (e.g., PET and MRI) and optical (e.g., scattering, fluorescence, confocal, and multiphoton) techniques can be used for visualizing only single static or slowly migrating cells [8–10]. To detect fast moving cells in blood and lymph flows, a number of methods providing *in vivo* FC have been developed [11–21]. In particular, the principle of FC has been adapted to the *in vivo* monitoring of labeled cells in ear blood vessels, and a few modifications of *in vivo* flow cytometers that are capable of real-time confocal detection of fluorescently labeled cells in both the arterial and venous circulation of small animals, have been built [12–14].

The alternative photothermal (PT) and photoacoustic (PA) techniques for *in vivo* blood FC, which do not require cell labeling and are not sensitive to light scattering and autofluorescence background, have also been recently suggested [15–17]. These techniques have potential application in the study of normal and abnormal cells in their native condition in blood or lymph flows *in vivo*, including molecular imaging, studying the metabolism and pathogenesis of diseases at a cellular level, and monitoring and quantifying metastatic and apoptotic cells and/or their responses to therapeutic interventions (e.g., drug or radiation).

Video microscopy and particle tracking methods adapted and integrated with an ultrahigh-speed imaging camera were used to measure lymph velocities throughout the entire lymphatic contraction cycle in the rat mesentery [18–23]. *In vivo*, label-free, high-speed (up to 10 000 with the potential for 40 000 fps), high-resolution (up to 300 nm) optical imaging of circulating individual erythrocytes, leukocytes, and platelets in fast blood flow has been developed [22]. Different potential applications of *in vivo* digital video microscopy include visualization of circulating cells and their deformability in lymph and blood flows and the study of the kinetics of platelets and leukocyte rolling, with high sensitivity and resolution.

Multiphoton fluorescence flow cytometry and its confocal and fiber-optic modifications hold a great promise for *in vivo* monitoring of multiple circulating cell populations in blood and lymph flows by exciting and detecting the emission from multiple fluorophores, such as fluorescent proteins and exogenous chromophores, important for multilabeling of cells of interest [24, 25].

There are many books on cytometry published since the 1980s (see, for example, the list on the web site [1]). They could be classified as books on general flow cytometry and cell sorting, clinical cytometry, and microscopic and imaging cytometry. The most recent and comprehensive are Refs [2, 3, 5, 8–10, 26–30]. The book by Shapiro [5] is the fourth edition on classic flow cytometry. This is one of the best textbooks, and covers well the field of practical flow cytometry prior to 2003

well. Recently, two books on flow cytometry and cellular diagnostics have been published in German and French [26, 27]. Both books were written and edited by well-known experts in the field. Karger has published the English translation of the German book edited by Ulrich Sack, Attila Tárnok, and Gregor Rothe, which is a bestseller in German [28]. Practical cytometry protocols have been given in the third edition of the book edited by Michael G. Ormerod [29]. The recent second edition of the book by Wojciech Gorczyca is more clinically and practically oriented [30]. Michael G. Ormerod has also designed an introductory book “to give that knowledge, aiming at people coming to flow cytometry for the first time,” in which all the major applications in mammalian biology are covered [31].

While the above-mentioned books describe clinical diagnostic methods and receipts of their applications, the current book is more research oriented and opens new perspectives in the development of flow cytometry for *in vivo* studies. It contains novel results of basic research on light scattering by different types of cells, which are very important for the improvement of already existing technologies and for designing new technologies in optical cytometry. The recently invented and fast-moving-to-practice methods of *in vivo* flow cytometry, based on ultrafast video and phase intra-vital microscopy and light scattering, diffraction, speckle, fluorescence, multiphoton, Raman, photothermal, and photoacoustic phenomena, are presented in the book.

In Chapter 1, *Perspectives in Cytometry* by Anja Mittag and Attila Tárnok, in addition to definitions, historical aspects, and the importance of cytometry in the development of biology and medicine, its prospective application as a science and diagnostic tool are discussed – in particular, for comprehensive analyses, on the basis of the simultaneous detection of several parameters, of up to millions of individual cells in one sample.

Chapter 2 by Herbert Schneckenburger *et al.*, *Novel Concepts and Requirements in Cytometry*, presents slide-based cytometry techniques and the concepts of high content screening (HCS) where detailed information is accumulated from a single cell or examination of multicellular spheroids where 3D detection methods are required. These techniques include microscopic setups, fluorescence reader systems, and microfluidic devices with micromanipulation, for example, cell sorting.

In Chapter 3 by Stoyan Tanev *et al.*, *Optical Imaging of Cells with Gold Nanoparticle Clusters as Light Scattering Contrast Agents: A Finite-Difference Time-Domain Approach to the Modeling of Flow Cytometry Configurations*, a brief summary of different formulations of the finite-difference time-domain (FDTD) approach is presented in the framework of its strengths, for cytometry in general and for potential applications in *in vivo* flow cytometry based on light scattering, including nanoscale targets. This chapter focuses on comparison of light scattering by a single biological cell alone under controlled refractive index matching conditions and by cells labeled using gold nanoparticle clusters. The optical phase contrast microscopy (OPCM) is analyzed as a prospective modality for *in vivo* flow cytometry.

In Chapter 4 by Valeri P. Maltsev *et al.*, *Optics of White Blood Cells: Optical Models, Simulations, Experiments*, a state-of-the-art summary of analytical and numerical simulating methods and experimental approaches for precise description and

detection of elastic light scattering from white blood cells (WBCs) are presented. The discussion of the instrumental tools for measurement of light scattering lays emphasis on scanning flow cytometry. This chapter gives some basis for understanding the methods, techniques, and experimental results presented in the following chapters, as it presents solutions for the inverse light-scattering problem to obtain cellular characteristics from light scattering data.

The optical properties of blood are discussed in Chapter 5 by Martina Meinke *et al.*, *Optical Properties of Flowing Blood Cells*. Authors use the transport theory accounting for the multiplicity of light scattering events, where the optical properties of blood are described by the absorption and scattering coefficients and the anisotropy factor. The double integrating sphere measurement technique combined with inverse Monte Carlo simulation is applied for extraction of the optical parameters of undiluted blood. It is shown that the influence of the shear rate and osmolarity have to be taken into account when the blood is prepared *ex vivo* and the physiological environment cannot be ensured.

In Chapter 6, *Laser Diffraction on RBC and Deformability Measurement* by Alexander V. Priezhev *et al.*, RBC shape variability and deformability as intrinsic properties, their strong relation to RBC aggregation and blood rheology, and the determination of the general hemorheologic status of human organism are considered. It is shown that laser diffraction can be efficiently applied to quantitatively assess the deformability properties of RBC in the blood of a particular individual. The theoretical basis of diffractometry and implementation of particular experimental techniques to experimental and clinical measurements, as well as potentialities and pitfalls of the technique are discussed.

The principles and fundamentals of flicker spectroscopy as a quantitative tool to measure static and dynamic mechanical properties of composite cell membrane are presented in Chapter 7, *Characterization of Red Blood Cells Rheological and Physiological State Using Optical Flicker Spectroscopy* by Vadim L. Kononenko. These mechanical properties are associated with cell membrane and cytoplasm molecular organization and composition and cell metabolic activity and could be characteristic not only for RBC, but for other blood cell types as well. Microscope-based flicker spectroscopy technique in combination with quantitative phase imaging and fluorescence microscopy can be easily integrated into the slide-based cytometry arrangement. As the author states, the approximate models developed are good, but not enough to reconstruct precisely the details of erythrocyte cell membrane mechanical properties; thus a more advanced theory of flicker spectroscopy is needed.

Chapter 8, *Digital Holographic Microscopy for Quantitative Live Cell Imaging and Cytometry*, by Björn Kemper and Jürgen Schnakenburger, demonstrates the principles and applications of quantitative cell imaging using digital holographic microscopy (DHM). The quantitative phase contrast imaging, cell thickness determination, multifocus imaging, and 2D cell tracking provided by DHM show that it is a suitable method for the label-free characterization of dynamic live cell processes involving morphological alterations and migration and for the analysis of cells in 3D environments. Examples and illustrations of applicability of the technique in

tumor cell biology and for the development of improved systems for drug and toxicity testing are presented.

Chapter 9 by József Bocsi *et al.*, *Comparison of Immunophenotyping and Rare Cell Detection by Slide-Based Imaging Cytometry and by Flow Cytometry*, allows one to get answers on the following questions: are flow cytometry (FC) and slide-based cytometry (SBC) comparable? What is the type of cytometer and analysis technique that should be chosen for the given biological problem to be solved? Answers are illustrated by applying scanning fluorescence microscope (SFM) to determine of CD4/CD8 T cell ratio, laser scanning cytometer (LSC) to multiparametric leukocyte phenotyping and apoptosis analysis on the basis of DNA content measurements, and SFM and LSC to rare and frequent tumor cell detection.

A brief overview and discussion of recent progress in microfluidic flow cytometry, including the main components of full scale flow cytometers, containing systems for fluidic control, optical detection and cell sorting, each of which are being developed into on-chip microfluidic platforms, are given by Shawn O. Meade *et al.* in Chapter 10, *Microfluidic Flow Cytometry: Advancements Toward Compact, Integrated Systems*.

In Chapter 11 by Xin-Hua Hu and Jun Q. Lu, *Label-Free Cell Classification with a Diffraction Imaging Flow Cytometer*, aiming at the accurate modeling of light scattering from biological cells with realistic cell structures and the development of a high contrast diffraction imaging flow cytometer for experimental study, the authors are focused on the application of the FDTD method for modeling of coherent light scattering from cells. Numerical and experimental results are presented and their implications to future improvement of the flow cytometry are discussed.

In Chapter 12 by Rabindra Tirouvanziam *et al.*, *An Integrative Approach for Immune Monitoring of Human Health and Disease by Advanced Flow Cytometry Methods*, the authors show key steps to move past the current limitations and truly enable the use of advanced flow cytometry tools for human research, promoting simplified, low-cost, and better standardized methods for sample collection, highlighting the enormous opportunities for research on reagents available for advanced flow cytometry analysis of human samples, and novel insights into relations of human immunity with age, gender, ethnicity, environmental exposure, health conditions, and therapies.

R. Dasgupta and P.K. Gupta, in Chapter 13, *Optical Tweezers and Cytometry*, give a brief introduction to optical tweezers and an overview of their use in cytometric applications, including measurements of viscoelastic properties of cells, in particular RBC, and Raman spectroscopic studies at single cell level. A few examples illustrating the potential of this approach for cytometric applications are also presented.

Chapter 14 by Valery V. Tuchin *et al.*, *In vivo Image Flow Cytometry*, presents one of the novel approaches in flow cytometry – *in vivo* video imaging digital flow cytometry. The fundamentals and instrumentation of video imaging flow cytometry, as well as spatial and temporal resolution of the method, are discussed. Experimental animal models, data on imaging and detection of individual cells in lymph and blood flows, and cell velocity measurements in lymph and blood vessels are presented and discussed. Intravessel RBC deformability measurement, monitoring of intralymphatic cell aggregation, and many other cell interaction

phenomena are demonstrated and quantified. Perspectives of the technique for disease diagnostics and monitoring and cell flow response on drugs, pollutants, and toxins are shown.

Chapter 15 by Stephen P. Morgan and Ian M. Stockford, *Instrumentation for In Vivo Flow Cytometry: A Sickle Cell Anemia Case Study*, discusses label-free monitoring of the properties of circulating blood cells for the *in vivo* monitoring of sickle cell anemia. For discriminating sickled RBCs in a background of normal cells, absorption measurements associated with sickle cell lower oxygen saturation and polarization measurements to identify their polymerization ability via cell adhesion to the vascular walls and, thus, more slow flow, are used. Illumination methods overcoming surface reflections, such as orthogonal polarization spectral imaging, dark field epi-illumination, and sidestream dark field illumination, are analyzed. In humans blood cell imaging has been performed either on the lower lip or under the tongue where the superficial mucosal tissue above the microcirculation is thinner than at other sites on the body. All steps of clinical instrumentation design, starting from discussion of the clinical needs for the measurements, the illumination and detection requirements, image processing methods for correction of image distortions, and a Monte Carlo model of the image formation process, up to engineering of the clinical prototype and presentation of clinical results are highlighted by the authors.

Accounting for the clinical importance of detection and quantification of circulating tumor cells (CTCs) for cancer diagnosis, staging, and treatment, in Chapter 16, *Advances in Fluorescence-Based In Vivo Flow Cytometry for Cancer Applications*, Cherry Greiner and Irene Georgakoudi, review the principles and instrumentation designs of fluorescence-based *in vivo* flow cytometry (IVFC) and present data on the *in vivo* quantification of CTCs. The confocal and multiphoton microscopic techniques and systems adapted for the detection of fluorescently labeled CTCs in blood vessels are described. The noninvasive nature of IVFC systems and their capability to provide sensitive, continuous and dynamic monitoring of CTCs in blood flow are proved.

Chapter 17, *In Vivo Photothermal and Photoacoustic Flow Cytometry* by Valery V. Tuchin *et al.*, is devoted to presentation of the prospective approaches of IVFC that use laser-induced photothermal (PT) and photoacoustic (PA) effects. The authors analyze in detail integrated IVFC techniques combining a few different methods, such as PT imaging conjugated with thermo-lens and PA imaging, transmittance digital microscopy, and phase-sensitive and fluorescence imaging. The unique capabilities of the PT/PAFC (photoacoustic flow cytometry) technique for IVFC are illustrated in many examples of *in vivo* and *ex vivo* studies within lymph and blood vessels of animal models. Data on cell velocity measurements, detection, and real-time monitoring of circulating blood and lymph cells, bacteria, CTCs, contrast agents, and nanoparticles, and on quantification of cell interactions are presented. Perspectives of PT/PAFC technique for early diagnostics of cancer are discussed.

Martin J. Leahy and Jim O'Doherty, in Chapter 18, *Optical Instrumentation for the Measurement of Blood Perfusion, Concentration, and Oxygenation in Living Microcirculation*, compare the operation of an established microcirculation imaging technique,

such as laser Doppler perfusion imaging (LDPI), which, for example, has been shown to accurately assess burn depth, with laser speckle perfusion imaging (LSPI) and tissue viability imaging (TiVi) in human skin tissue using the occlusion and reactive hyperaemia response. On the basis of the presented experimental data they conclude that LSPI and TiVi are both welcome tools in the study of the microcirculation, but care must be taken in the interpretation of the images since blood flow velocity and blood concentration in tissue are essentially different parameters.

In Chapter 19, *Blood Flow Cytometry and Cell Aggregation Study with Laser Speckle Contrast Imaging (LSCI)* by Qingming Luo *et al.*, the fundamentals and instrumentation of laser speckle contrast imaging (LSCI) are analyzed with a discussion of important imaging parameters for the optimal imaging conditions. Some recent advancements, such as spatio-temporal algorithm for laser speckle contrast analysis and fast blood flow visualization using GPU (Graphics Processing Unit), are overviewed. The application of LSCI for investigation of RBC aggregation is discussed.

Chapter 20, *Modifications of Blood Optical Properties during Photodynamic Reactions In Vitro and In Vivo*, by Alexandre Douplik *et al.*, describes photodynamic reactions where blood cells are involved. Change in blood properties on light delivery and modification of photosensitizer (PS) optical properties on interaction with blood at photodynamic therapy (PDT) are considered. The blood cell uptake of PSs and modification of blood optical properties caused by PDT reactions *in vitro* and *in vivo* are analyzed. The authors of the chapter believe that IVFC can be applied to study PDT-induced processes related to blood and blood cells.

As it follows from the above, this book is focused on state-of-the-art research in a novel field, noninvasive *in vivo* cytometry, and its applications, with particular emphasis on the novel biophotonic methods, disease diagnosis, and monitoring of disease treatment at single cell level in stationary and flow conditions. However, discussions of advanced methods and techniques of classical flow cytometry are also presented. The use of photonic technologies in medicine is a rapidly emerging and potentially powerful approach for disease detection and treatment. This book seeks to advance scholarly research that spans from fundamental interactions between light, cells, vascular tissue, and cell labeling particles, to strategies and opportunities for preclinical and clinical research. General topics include light scattering by cells, fast video microscopy, polarization, laser scanning, fluorescence, Raman, multiphoton, photothermal, and photoacoustic methods for cellular diagnostics and monitoring of disease treatment in living organisms. Specific topics include optics of erythrocytes, leukocytes, platelets, and lymphocytes; novel photonic cytometry techniques; *in vivo* studies using animal models; *in vivo* cytometry techniques used in humans (mucosal, nail bed, and skin); detection of metastatic cancer cells and labeling of nanoparticles in blood and lymph microvessels; immune monitoring of human health; cytomics in regenerative/predictive medicine; comparison of laser scanning slide-based and flow cytometry, and so on.

The book is for research workers, practitioners, and professionals in the field of cytometry. Advanced students (MS and Ph.D.) as well as undergraduate students specialized in biomedical physics and engineering, biomedical optics and biophotonics, and medical science may use this book as a comprehensive tutorial helpful in

the preparation of their research work and diploma. Scientists or professionals and students in other disciplines, such as laser and optical engineering and technology, spectroscopy, tomography, developmental and other directions of biology, tissue engineering, and different specialties in medicine, are also potential readership.

This book represents a valuable contribution by well-known experts in the field of photonic cytometry with their particular interest in a variety of advanced cytometry problems, including *in vivo* flow cytometry. The contributors are drawn from Canada, China, Denmark, Germany, India, Ireland, Russia, The Netherlands, UK, and the USA. I greatly appreciate the cooperation and contributions of all authors in the book, who have done great work in the preparation of their chapters.

It should be mentioned that this book presents results of international collaborations and exchanges of ideas among many research groups participating in the book project. This book project was supported by many international grants, which are credited in the particular chapters. Here, I would like to mention only a few, PHOTONICS 4 LIFE, which is a consortium of a well-balanced pan-European dimension. The inclusion of the members of this consortium in this book is of great significance, encompassing five chapters. My own work on the book was supported by grants 2.1.1/4989 and 2.2.1.1/2950 of RF Program on the Development of High School Potential and RF Governmental contracts 02.740.11.0484, 02.740.11.0770, and 02.740.11.0879 of The Program “Scientific and Pedagogical Personnel of Innovative Russia.”

I am grateful to Valerie Moliere for her suggestion to publish this book and help on project activation and to Ulrike Werner for the technical editing of the book and communication with the contributors.

I would like to thank all those authors and publishers who freely granted permissions to reproduce their copyrighted works.

I greatly appreciate the cooperation, contributions, and support of all my colleagues from the Optics and Biophotonics Chair and Research-Educational Institute of Optics and Biophotonics of the Physics Department of Saratov State University and the Institute of Precise Mechanics and Control of the Russian Academy of Science.

I express my gratitude to my family, especially to my wife Natalia and grandchildren Dasha, Zhenya, Stepa, and Serafim for their indispensable support, understanding, and patience during my writing and editing of this book.

August 2010

Saratov

References

1. Robinson, J.P. (2011) *Reference Books in Cytometry*, Purdue University Cytometry Laboratories, <http://www.cyto.purdue.edu/flowcyt/books/bookindx.htm>, February 21, 2011.
2. Melamed, M.R., Lindmo, T., and Mendelsohn, M.L. (eds) (1990) *Flow Cytometry and Sorting*, 2nd edn, Wiley-Liss, New York.
3. Hudnall, S.D. (ed.) (2000) *Introduction to Diagnostic Flow Cytometry: An Integrated*